



SUMMIT FRS W/TABLE  
143 SQ. FT.

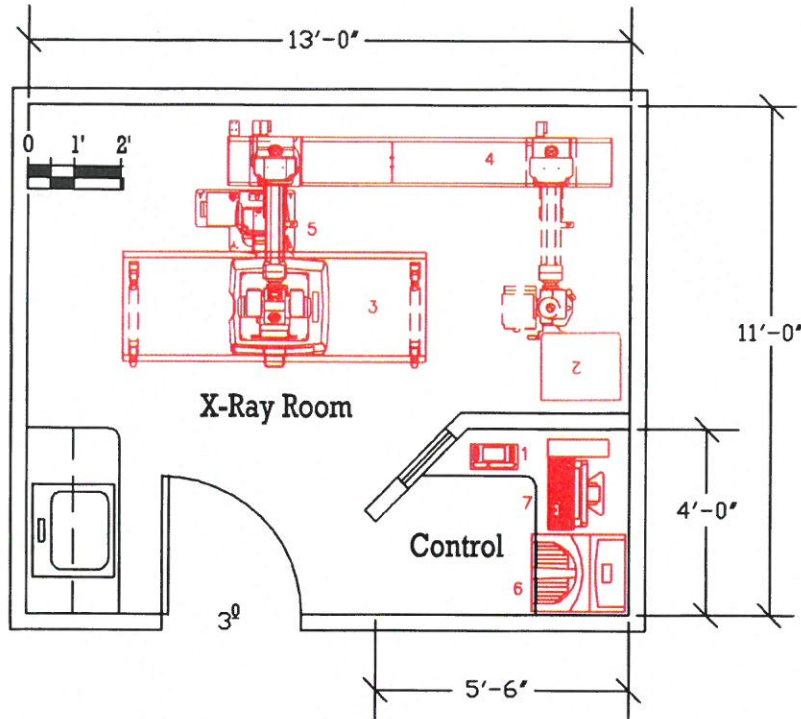

MINIMUM ROOM SIZE  
(DOES NOT MEET ADA REQUIREMENTS)



EQUIPMENT SCHEDULE

NOTES / POWER

ITEM	DESCRIPTION	WIDE	DEEP	HIGH	LBS
1	SUMMIT OPERATOR CONSOLE	12"	7"	3"	6
2	SUMMIT GENERATOR CABINET	21"	18"	37"	209
3	SUMMIT MOBILE TABLE	79"	29"	28"	198
4	SUMMIT FRS TUBE STAND	100"	57"	85"	XXX
5	SUMMIT FRS IMAGE RECEPTOR	35"	46"	56"	XXX
6	TYPICAL CR READER	20"	24"	14"	62
7	TYPICAL CR WORKSTATION	28"	16"	21"	65

- ALL SPECIFICATIONS, AND SPACE ILLUSTRATIONS ARE SHOWN GENERICALLY. CONTACT LOCAL SUMMIT REPRESENTATIVE FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED CEILING HEIGHT: 9' -0"
- SUGGESTED AMBIENT ROOM REQUIREMENTS ARE 41 DEGREES TO 86 DEGREES F. AT 10% TO 75% R.H. (NON-CONDENSING). THE BTU/HR. RATINGS LISTED BELOW ARE ESTIMATIONS BASED ON AN AVERAGE HOURLY DUTY CYCLE AND STANDBY MODES OF EQUIPMENT OPERATION:  

EXAM ROOM	1,417 --
CONTROL AREA	1,530 --
TOTAL	2,947 BTU/HR.
- ALL COUNTER TOPS AND CABINETS SHOWN TO BE DESIGNED, SUPPLIED, AND INSTALLED BY CUSTOMER/CONTRACTOR.
- VIEW WINDOW IN CONTROL AREA TO BE DESIGNED, SUPPLIED, AND INSTALLED BY CUSTOMER/CONTRACTOR.

**mdi**  
MEDICAL DESIGN, INC.

THESE DRAWINGS ARE SUBMITTED TO SUGGEST LOCATION OF DIAGNOSTIC IMAGING EQUIPMENT AND ASSOCIATED APPARATUS. SOME ITEMS SHOWN ARE OPTIONAL. IN PREPARING THIS DRAWING, EVERY EFFORT HAS BEEN MADE TO CONFORM DETAILS TO THE EQUIPMENT EXPECTED TO BE INSTALLED. THESE DRAWINGS ARE NOT TO BE USED FOR CONSTRUCTION PURPOSES, AND THE PREPARER CANNOT ACCEPT ANY LIABILITY FOR DAMAGES RESULTING THEREFROM. CONSTRUCTION DRAWINGS ARE TO BE PREPARED BY PURCHASER'S ARCHITECT OR CONTRACTOR.

DWG. # **FRS W/TABLE**  
DATE: **09/04/13**  
SHEET: **1 OF 1**